



校准证书

CALIBRATION CERTIFICATE



扫一扫验真伪

1GA25060919892-0005A

校验码:A251CC77

证书编号:

Certificate No.

委托方:

Client

Desert Aire

委托方地址:

Address

N120 W18485 Freistadt Road, Germantown, WI 53022, USA (Post code: 53022)

仪器/样品名称:

Description

Test Finger Nail of IEC 60335-1 Figure 7

型号/规格:

Model/Type

SMT-335F7

制造厂商:

Manufacturer

LISUN GROUP

出厂编号:

Serial No.

LS2025026305

管理号:

Asset No.

样品接收日期:

Date of Receipt

2025-06-09

Y M D

结果:

Conclusion

按实测结果使用,见报告内页(Use according to the measured results, See the page of the report)

校准日期:

Date of Calibration

2025-06-11

Y M D

建议下次校准日期:

Due Date

2026-06-10

Y M D

校准:

Calibration by

黄子铭

黄子铭

审核:

Inspected by

胡中兴


胡中兴

授权签字人:

Approved Signatory

韦寿前

韦寿前

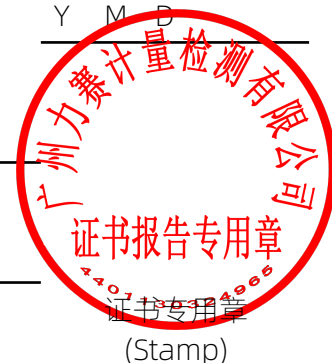

本实验室地址: 广东省广州市番禺区石碁镇农科所南街8号

Address: No.8.South Street Shi Ji Institute Guangzhou.Guangdong.China

联系电话(Tel): 020-31134076

投诉电话(CT): 020-39969860

传真(Fax): 020-39969986

邮政编码(Post): 511400

公司网址(Web): www.lisaitest.com

电子邮件(E-mail): cal@lisaitest.com

我司电子证书具备网站/微信公众号查验(二维码扫码查验)、校验码、电子签章(查验内容是否修改且一致)三重防伪验证。



校准说明

DIRECTIONS OF CALIBRATION

证书编号:
Certificate No.



1GA25060919892-0005A
校验码:A251CC77

本实验室质量管理体系符合ISO/IEC17025标准要求。

The quality system is in accordance with ISO/IEC17025.

1. 本实验室出具的数据均可溯源至国际单位制(SI)。

All data issued by this laboratory are traceable to International System of Units(SI)

2. 证书中最大允许误差、判定结果仅供参考,其中"P"代表"合格","F"代表"不合格","N/A"代表"不适用"。

使用人员应结合实际测量需求,评估测量不确定度对符合性评定的影响。

MPE & judgement result in the datasheet is only for reference,"P" represents "Pass" and "F" represents "Fail" and "N/A" represents "Not Applicable".Where as users should evaluate the effects of MU of calibration results on conformance assessment by actual measurement.

3. 本证书编号具有唯一性,后缀若带有"A~Z"的证书为替换证书,自发出后原证书即刻作废。

Each certificate has a unique number,The suffix of "A~Z" will be added to the number as a replacement of the old version. The original certificate will be officially invalid once the new certificate number is issued.

4. 校准地点、环境条件。(Place and environmental condition of the Calibration).

广州实验室(101精测室)

温度(Temperature): 20.4°C 相对湿度 (Relative Humidity): 58 %

5. 未加盖“证书报告专用章”无效,报告无校准或检测、审核、授权签字人签章无效。

The report is invalid without the official stamp, report is invalid without 'report stamp', The report is invalid without the signatures of Approval and Reviewer.

6. 本次校准的技术依据及CNAS认可范围,超出范围的内容未被认可。详细认可范围请查看CNAS网站中注

册编号为L7127的证书附件。(Reference documents and accredited scope by CNAS for the Calibration beyond which isn't accredited. Please see the attachment of certificate No.L7127 on CNAS website for details.)

JJG 455-2000 工作测力仪检定规程 V. R. of Working Dynamometers

JJF(新)68-2021 一维、二维几何尺寸测量校准规范 Calibration specification for one-dimensional and two-dimensional geometric dimension measurement

7. 计量溯源性声明:Measurement traceability declaration:

被校器具: Test Finger Nail of IEC 60335-1 Figure 7; 被校器具 → 数显推拉力计 → 力值砝码(9个) → 广州市番禺质量技术监督检测所; 被校器具 → 数显卡尺 → 卡尺量块 → 华南国家计量测试中心

8. 本次校准使用的主要计量标准器具。(Main standards of measurement used in the Calibration).

名称/型号 Equipment/Model	出厂编号 Serial No.	证书号/有效期 Certificate No./ Due Date	溯源机构 Traceability Institute	技术特征 Technique Character
数显推拉力计/ SBG-10C	1C060111	3GC240702111126-213 0 / 2025-07-29	广州力赛计量检测有限公司	0.5级
万能工具显微镜/ (200×100)mm	3875	CYY202500409 / 2026-04-27	华南国家计量测试中心	MPE: ± (1+L/100)μm; L: mm
数显卡尺/ (0~300)mm	K18A305749	3GC250102161689-750 9 / 2026-01-22	广州力赛计量检测有限公司	(0~70) mm, MPE=±0.02mm; (> 70~200) mm, MPE=±0.03mm; (> 200~300) mm, MPE=±0.04mm



证书编号:
Certificate No.




1GA25060919892-0005A
校验码:A251CC77

1、外观以及一般性检查：正常
In view of External and Generality check : Pass

2、尺寸校准(Dimensional calibration):

2.1、示意图 (Diagram)

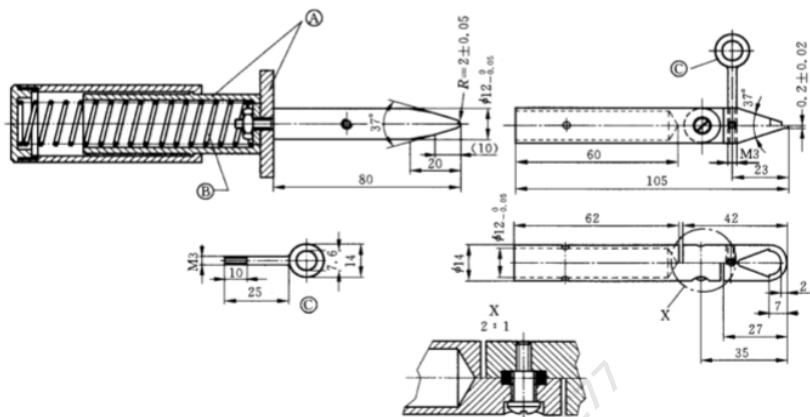

关键词
A:绝缘材料;
B:弹簧 φ18 mm;
C:拉环。

图 7 试验指甲

2.2、尺寸校准(Dimensional calibration):

	标称值 Nominal (mm)	实测值 Measured (mm)	U (k=2) (mm)	技术要求 Requirement (mm)	结 论 Conclusion (Pass/Fail)
1	2	2.03	0.01	1.95 ~ 2.05	P
	80	80.03	0.04	79.80 ~ 80.20	P
	10	9.97	0.03	/	/
	20	20.03	0.03	/	/
	12	11.98	0.01	11.95 ~ 12.00	P
	0.2	0.215	0.006	0.18 ~ 0.22	P
	23	23.03	0.03	/	/
	60	59.89	0.04	/	/
	105	105.23	0.04	/	/
	2	1.98	0.03	/	/
	7	6.99	0.03	/	/



证书编号:
Certificate No.



1GA25060919892-0005A
校验码:A251CC77

2.2、尺寸校准(Dimensional calibration): 续上

	标称值	实测值	U	技术要求	结 论
	Nominal	Measured	(k=2)	Requirement	Conclusion
	(mm)	(mm)	(mm)	(mm)	(Pass/Fail)
	27	27.02	0.03	/	/
	35	35.05	0.03	/	/
	42	42.01	0.03	/	/
	62	62.02	0.04	/	/
2	12	11.99	0.01	11.95 ~ 12.00	P
	14	13.97	0.03	/	/
拉环A	14	13.97	0.03	/	/
拉环A	7.6	7.63	0.03	/	/
拉环B	14	13.97	0.03	/	/
拉环B	7.6	7.62	0.03	/	/
	(°)	(°)	(°)		
1	37	36.9	0.3	/	/
2	37	36.9	0.3	/	/

3、推力校准 (Thrust calibration) :

标称值	实测值	U
Nominal	Measured	(k=2)
(N)	(N)	(N)
10	9.8	0.3
20	19.5	0.6
30	29.3	0.9
40	39.3	1.2
50	48.9	1.5

注：技术要求由客户提供
Note: Technical requirements to be provided by the customer



广州力赛计量检测有限公司

Guangzhou LiSai Metrology & Test Co., Ltd.



证书编号:

Certificate No.



1GA25060919892-0005A

校验码:A251CC77

附: 关于测量结果不确定度的说明:

appendix: Directions of uncertainty in the calibration

1.依据(Reference document)

JJF 1059.1-2012 测量不确定度评定与表示

(JJF 1059.1-2012 Evaluation and Expression of Uncertainty in Measurement)

2.本报告给出的扩展不确定度是由合成标准不确定度乘以包含概率约为95%时对应的包含因子k得到的。

The expanded uncertainty given in this report is obtained by multiplying the combined standard uncertainty by the corresponding coverage factor k when the coverage probability of about 95%.

-----以下空白(The below is blank)-----

校验码: A251CC77

